



**HAL**  
open science

## Ingestible sensors correlate closely with peripheral temperature measurements in febrile patients

Fanyu Huang, Chloe Magnin, Philippe Brouqui

► **To cite this version:**

Fanyu Huang, Chloe Magnin, Philippe Brouqui. Ingestible sensors correlate closely with peripheral temperature measurements in febrile patients. *Journal of Infection*, 2020, 80 (2), pp.161-166. 10.1016/j.jinf.2019.11.003 . hal-02496177

**HAL Id: hal-02496177**

**<https://amu.hal.science/hal-02496177>**

Submitted on 7 Mar 2022

**HAL** is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.



Distributed under a Creative Commons Attribution - NonCommercial 4.0 International License

1 **Agreement between Sensors and Peripheral Temperature**

2 **Measurements in Febrile Patients**

3 **Running Title: Temperature sensors and febrile patients**

4 Fanyu Huang RN MSc, Chloe Magnin MSc, Philippe Brouqui MD PhD

5 Department of Research Microbes Evolution Phylogeny and Infections (MEPHI), The Institute  
6 for development research (IRD), University Hospital Institute-Mediterranean infection, Aix  
7 Marseille University, Marseille, France

8 \*Corresponding author: Philippe Brouqui, Fanyu HUANG

9 **Full address:** Institut Hospitalo Universitaire Méditerranée Infection, 19-21 Boulevard Jean  
10 MOULIN, 13005, Marseille, France

11 Email: [philippe.brouqui@univ-amu.fr](mailto:philippe.brouqui@univ-amu.fr)

12 [fanyu.huang@etu.univ-amu.fr](mailto:fanyu.huang@etu.univ-amu.fr)

13

14

# 1 **Introduction**

2 Measuring human body temperature has been recognised as a major clinical sign for more than  
3 150 years. Body temperature influences clinical management decisions and the diagnosis of  
4 certain diseases, but is also an important indicator for estimating body metabolism, body  
5 movement and physical activity [1,2].

6 When an infectious disease occurs, fever is one of many important indicators; the febrile  
7 response means that the body is fighting the infection [3]. It is referred to as a “fever” when the  
8 core temperature (head and thorax) is above 38.3°C [4]. The normal core temperature range is  
9 between 36.5 °C and 37.3 °C; the periphery is 2 to 4 °C lower than that of the core [2].

10 There are several non-vascular methods to assess core temperature, including oesophageal and  
11 urinary bladder measurements [5]. However, these non-vascular methods are invasive because  
12 they require the use of a catheter and measuring rectal temperature creates a sense of  
13 humiliation and discomfort. On the other hand, peripheral temperature measurements, such as  
14 axillary temperature, tympanic temperature and temporal temperature are non-invasive but  
15 may underestimate the core temperature and increase contact transmissions [6]. Peripheral  
16 temperature measurements could be influenced by the following reasons: patient activity, basal  
17 metabolism rate, fat mass, skin blood flow, measurement errors (incorrect thermometer  
18 positioning) and ambient temperature.

19 Non-contact methods are particularly valued in highly contaminated environments. The ideal  
20 measurement method must be accurate, precise and non-invasive; in addition, the ideal site for  
21 measurements must meet the following requirements: not be influenced by ambient  
22 temperature; reflect the core temperature quantitatively and quickly; and be as non-invasive as  
23 possible [7].

24 In clinical practice, axillary thermometers, tympanic and temporal infrared thermometers are  
25 used frequently. However, a recent meta-analysis showed that measurements taken by  
26 peripheral thermometers were highly variable. This analysis included 75 studies, involving  
27 8,682 patients from 21 countries. This analysis concluded that most peripheral thermometers  
28 were not accurate enough to be considered as clinically acceptable core temperature  
29 measurements [8].

30 Ingestible telemetric body core temperature sensors have been extensively used in sports  
31 medicine specially to track core temperature during exercises. These non-invasive temperature  
32 measurement methods have been established as valid index of core temperature in several  
33 studies and have been suggested some time ago as having a good potential for ambulatory  
34 monitoring [9,10]. A recent study compared four different models of ingestible capsules and  
35 demonstrated the excellent consistency and accuracy of this device [11]. In clinical medicine  
36 and, specifically, in infectious diseases, measuring the temperature of bedridden patients is  
37 essential, yet takes nursing time and disturbs patients during the night. While ingestible  
38 telemetric body core temperature sensors have been shown to correlate with rectal temperature  
39 [12], they have not yet been compared to routine temperature measurements in clinical care in  
40 patients with fever.

41 This study assessed the agreement between peripheral temperature measurements used in  
42 clinical practice (axillary, non-contact) and both skin temperature recorded by skin sensor and  
43 core temperature measurements taken by an ingestible capsule in a single cohort of febrile  
44 patients.

45

46

## 47 **Materials and methods**

### 48 **Study design**

49 This open-label study was conducted in the department of infectious diseases at the University  
50 Hospital Institute Méditerranée-Infection located in Marseille, France. All the procedures for  
51 this study were approved by the Ethics Committee of Sud-Méditerranée IV (N° 180204) and  
52 the study was registered on the French register for clinical trial (ANSM) under N° ID-RCB:  
53 2018-A0014748 and in the European clinical trials database EudraCT under number **2018-**  
54 **004812-23**. In accordance with medical research ethics, all participating patients are protected  
55 (in accordance with the principles that originate in the Declaration of Helsinki). Each eligible  
56 patient was included in the study after providing their written informed consent. Patients were  
57 informed by the investigator or co-investigator of the study to the extent possible, based on  
58 their understanding.

59 To measure axillary temperature, this study used a mercury-free thermometer (Geratherm®  
60 Classic medical thermometer, CE0197, certified by NF EN ISO 13485); a new sensor, the  
61 eTact® (BodyCap®, Caen, France) was used for skin temperature. An infrared thermometer  
62 was used for non-contact forehead measurement in this study (HYLOGY Non-contact Infrared  
63 Thermometer, Model: MD-H26, CE0123, US FDA approved).

64 An ingestible sensor (e-Celsius performance pill ®, BodyCap®, Caen, France) was used for  
65 core temperature measurement. This ingestible capsule is a class IIB medical device and holds  
66 certification ISO13 485 and the CE mark, providing continuous measurement of  
67 gastrointestinal temperature (more detail, see Supplementary Appendix User Guide e-  
68 CELSIUS Performance). All calibrations of the devices were performed by the manufacturer  
69 in the 2018 version [12].

## 70 **Subjects**

71 This study included all patients who presented fever upon admission. Most were patients  
72 with acute infectious diseases: pneumonia, urinary tract infections, soft tissue infections, and  
73 all types of fever could be included in this study. All participants were social security insurance  
74 beneficiaries aged 18 years or older.

75 The exclusion criteria included: 1) pregnant or lactating women, 2) patients with or presenting  
76 a risk of intestinal disorders that can lead to obstruction of the digestive tract, including  
77 diverticulitis, 3) patients with motility disorders of the gastrointestinal tract, 4) patients who  
78 had undergone surgical procedures in the gastrointestinal tract, 5) patients with known  
79 swallowing disorders, 6) patients who had to undergo MRI scans (and who should thus avoid  
80 strong electromagnetic fields during the period of use of the system), 7) patients weighing less  
81 than 40 kg and vulnerable persons.

## 82 **Study protocol**

83 During the study, we collected each the pathologies, demography, medical history and  
84 medications of each patient using a bedside recording system developed in the institute (Florea  
85 O, Boudjema S, Magnin C, Brouqui P, Dufour JC, manuscript in preparation).

86 For every patient participating in this study, temperatures were recorded over a 48-hour  
87 observation period with axillary and non-contact forehead temperature measured by a mercury-  
88 free thermometer and infrared thermometer every two hours (8.30am, 10.30am, 12.30pm,  
89 2.30pm, 4.30pm); skin temperature was measured by eTact patch every minute. The core  
90 temperature was measured by the ingestible capsule (BodyCap©) every five minutes.

91 Axillary temperature measurements were taken from the patient's left arm and environment  
92 temperature was kept at 25 °C (to minimise the influence of environment) and non-contact

93 forehead temperature measurements were measured 5cm in front of the central forehead. Both  
94 temperature measurements were recorded in the patient's case report, which was approved by  
95 the Independent Ethics Committee. The ingestible capsule and eTact temperature  
96 measurements were stored in the e-Viewer Performance monitor and eTact monitor, then  
97 transferred to a computer in Excel format and all data were analysed by SPSS21 and R 3.4.2  
98 (for Bland-Altman plot).

## 99 **Statistical analysis**

100 The primary objective was to assess the agreement and Intraclass Correlation Coefficients  
101 (ICC) between the different types of body temperature measurement devices: ingestible  
102 capsule, axillary, non-contact forehead and eTact (skin) temperature. The sample size  
103 requirement for assessing ICC is 22 subjects (with power = 80%; alpha = 0.05; p=0.4; three  
104 observations per subject and  $R_0$  was set at zero). The normality of distribution was assessed by  
105 analysis of Skewness and Kurtosis.

106 This study analysed the correlation coefficient ( $r$ ) between axillary temperature measurements  
107 and other temperature measurement devices. However, the assessment of the relationship  
108 between the two methods is insufficient to demonstrate the degree of agreement and their  
109 difference [13]. Consequently, to evaluate whether both methods give identical readings,  
110 assessing the agreement (concordance) between series of repeated quantitative variables, it is  
111 necessary to analyse the ICC. To calculate ICC, McGraw and Wong defined 10 forms of ICC  
112 based on three "models" (one-way random effects, two-way random effects, or two-way fixed  
113 effects) and two "types" (single rater/measurement or the mean of  $k$  raters/measurements). This  
114 study chose the two-way mixed-effects model because repeated measurements cannot be  
115 considered to be randomised samples. To complete the agreement analysis, the Bland-Altman  
116 plot was used to assess the mean difference and construct the limits of agreement [14,15].

## 117 **Results**

118 The inclusion period ran from April 2018 to June 2018, during which 77 febrile patients were  
119 admitted and hospitalised. A total of 26 patients were deemed eligible and participated in this  
120 study.

121 Failure to obtain informed consent was the major cause of exclusion (20.78%, n=16), eight  
122 eligible patients were not communicative, one was under guardianship, one was not conscious  
123 enough and six eligible patients refused to participate. The second most common cause for  
124 exclusion was the hypothetical requirement of MRI scans (15.58%, n=12). The third cause for  
125 exclusion was swallowing disorders (12.99%, n=10) and other disorders (12.99%, n=10). The  
126 last cause for exclusion was digestive system disorders (3.9%, n=3).

127 Table 1 reports the characteristics of the 26 patients: 12 females and 14 males, aged  $48.6 \pm 17.5$   
128 years old (mean  $\pm$  SD); their mean body weight was  $65.9 (\pm 13.66)$  kg and blood pressure was  
129  $118.6 (\pm 17.87) / 64.3 (\pm 12.98)$  mm Hg. The mean capsule transit time (during 48 hours of  
130 observation) was  $37.3 (\pm 14.8)$  hours. The shortest duration was four hours (one patient).

131 Following the collection body temperature measurements from four different devices over the  
132 48-hour observation period, Table 2 summarises the percentages of missing measurements,  
133 mean temperature, standard deviation, and maximum and minimum variable.

134 There is a 16.5% gap in temperature measurements for ingestible capsules. The main cause of  
135 these missing measurements was the evacuation of the capsule before the 48-hour observation  
136 period or a synchronisation problem between the monitor and the capsule (n=42, 11 patients).  
137 eTact patches had fewer missing measurements at only 11.8% due to battery shutdown (n=18,  
138 5 patients) or removal of the device by the patient (n=12, 2 patients). As for axillary and non-  
139 contact measurements, there was a missing measurement rate of 16.5% (n=42) and 15.3%

140 (n=39) respectively, due to the absence of the patients at the time of recording and during the  
141 weekend.

142 To highlight the usefulness of the ingestible capsule temperature measurements, Figure 1A  
143 indicates the time trend data of all measurements in one selected patient. Figure 1B indicates  
144 the time trend data of one patient with hypothermia.

145 The regression line between the axillary temperature measurements ( $T_{\text{axi}}$ ) and non-contact  
146 forehead temperature measurements ( $T_{\text{no-c}}$ ), ingestible capsule temperature measurements  
147 ( $T_{\text{cap}}$ ) as well as eTact temperature measurements ( $T_{\text{etac}}$ ) are shown in Figures 2. The coefficient  
148 ( $r$ ) between  $T_{\text{axi}}$  vs.  $T_{\text{no-c}}$  is 0.47 (95% IC: 0.36; 0.57,  $R^2=0.22$ ,  $p<0.001$ ) and coefficient ( $r$ ) is  
149 0.85 (95% IC: 0.81; 0.98,  $R^2=0.72$ ,  $p<0.001$ ) between  $T_{\text{axi}}$  vs.  $T_{\text{cap}}$ . The correlation between  $T_{\text{axi}}$   
150 vs.  $T_{\text{etac}}$  is coefficient ( $r$ ) =0.42 (95% IC: 0.30; 0.52,  $R^2=0.17$ ,  $p<0.001$ ). The ICC between  $T_{\text{axi}}$   
151 vs.  $T_{\text{no-c}}$  is 0.34 (95% IC: -0.18; 0.63); 0.87 (95% IC: 0.55; 0.94) between  $T_{\text{axi}}$  vs.  $T_{\text{cap}}$ ; and 0.12  
152 (95% IC: -0.09; 0.37) between  $T_{\text{axi}}$  vs.  $T_{\text{etac}}$ . Table 3 summarises the comparison of each  
153 correlation and agreement between the three different devices and the axillary temperature  
154 measurements.

155 We also assessed the correlation at the time of each recording (10 recordings in 48 hours); no  
156 statistically significant differences were found during the 48-hour observation period.

157 Finally, Table 4 summarises the details of the Bland-Altman plot. This table shows the mean  
158 difference of two paired of measurements as well as their standard deviation and the limits of  
159 agreement. The mean difference between  $T_{\text{axi}}$  vs.  $T_{\text{no-c}}$  is  $-1.18^{\circ}\text{C}$  with 95% limits of agreement  
160 of  $-2.96^{\circ}\text{C}$  to  $0.58^{\circ}\text{C}$ . The mean difference between  $T_{\text{axi}}$  vs.  $T_{\text{cap}}$  is  $0.48^{\circ}\text{C}$  with 95% limits of  
161 agreement of  $-0.60^{\circ}\text{C}$  to  $1.56^{\circ}\text{C}$ . The mean difference between  $T_{\text{axi}}$  vs  $T_{\text{etac}}$  is  $-4.23^{\circ}\text{C}$  with 95%  
162 limits of agreement of  $-7.22^{\circ}\text{C}$  to  $-1.23^{\circ}\text{C}$ . Figures 3 indicate the difference of two pairs of  
163 measurements.

## 164 **Discussion**

165 While pulmonary arterial blood temperature is considered to be the gold standard for measuring  
166 core temperature, this invasive method cannot be used in non-ICU febrile patients. Ingestible  
167 telemetric body core temperature sensors have been shown to correlate with rectal  
168 temperature[11,16]. Rectal temperature has widely been dismissed in clinical practice due to  
169 its invasiveness and discomfort. Axillary temperature measurement is currently the non-  
170 invasive measurement that reflects the best core temperature (axillary temperature plus 0.5°C)  
171 and has been recommended as the standard for neonatal care [1,17].

172 Several studies have shown that non-contact (forehead or temporal artery) temperature  
173 measurements are a reliable, comfortable and accurate option for measuring body temperature  
174 and screening for fever in the paediatric population [18–20], and they have been widely used  
175 in airports since the outbreak of severe acute respiratory syndrome (SARS) [21,22]. In 2004,  
176 the U.S. Food and Drug Administration (US FDA) approved the use of this thermometer in  
177 children [20]. However, some studies have shown this method is not clinically acceptable in  
178 adults [23–26].

179 In this study, the non-contact forehead temperature measurements show a weak uphill linear  
180 relationship ( $r=0.42$ ) and poor strength of agreement ( $ICC <0.40$ ) with axillary temperature  
181 measurements. The Bland-Altman plot shows that more than 95% of points are within the limits  
182 of agreement, but 95% of points show that the difference between the  $T_{axi}$  vs.  $T_{no-c}$  is lower than  
183 zero. The mean difference between  $T_{axi}$  vs.  $T_{no-c}$  is  $-1.18$  °C, which is higher than the clinically  
184 acceptable range ( $\pm 0.5$  °C). This method underestimates core temperature because non-contact  
185 forehead temperature measurements could be influenced by blood flow under the skin, body  
186 metabolic rate and the distance between the thermometer and forehead. Moreover, according  
187 to the Bland-Altman plot, the difference between the two temperature measurements increases

188 as the temperature increases. Therefore, this method is neither sufficiently reliable nor  
189 clinically acceptable for screening for fever in adult febrile patients.

190 Skin sensors (eTact patches) exhibit a weak uphill linear relationship ( $r=0.42$ ) and a poor  
191 strength of agreement ( $ICC < 0.40$ ) with axillary temperature measurements. Skin temperature  
192 can be influenced by many factors such as blood flow under the skin, the body's metabolic rate  
193 and ambient temperature [27]. Thus, this method was less consistent than the core temperature  
194 measurements (SD of eTact measurements was 1.84 and the SD of ingestible capsule  
195 measurements was 1.01). The Bland-Altman plot shows that 95% of points were within the  
196 limits of agreement, but many of the points were further from zero. The mean difference was -  
197 4.23 °C, as the theory indicated; the skin temperature was 2 to 4 °C below the core temperature.  
198 However, this method did not correlate well with the reference temperature, so it is not  
199 acceptable for fever screening.

200 In our study, the ingestible capsule shows a strong uphill linear relationship ( $r=0.85$ ) and an  
201 excellent degree of agreement ( $ICC > 0.77$ ) with the axillary temperature measurements.  
202 According to the Bland-Altman plot, 95% of points are within the limits of agreement, and the  
203 mean difference between  $T_{axi}$  vs  $T_{cap}$  is 0.48 °C, which is within the clinically acceptable range  
204 ( $\pm 0.5$  °C). This difference between axillary temperature measurements and temperature  
205 measurements of ingestible capsules is, as the theory indicates, in the range of 0.5 to 1°C.  
206 Compared to other core temperature measurement methods, the ingestible capsule is less  
207 invasive and more comfortable method for patients. This method produces continuous body  
208 temperature measurements during gastro-intestinal transit. However, cold or hot food and drink  
209 intake can influence capsule temperature measurements[28]. According to Domitrovich *et al.*  
210 (2010), measurements of ingestible capsules are reliable after only 40 minutes of ingestion  
211 (when the sensor passes the stomach) [29]. In our study, we therefore took this constraint into  
212 account when analysing the data. Ingestible temperature sensors are an easy way to follow and

213 monitor core temperature; it has been reported that continuous core temperature measurements  
214 help to predict the early diagnosis of hospital-acquired sepsis [30]. Continuous core  
215 temperature measurements could offer a different perspective on patterns of fever and detect  
216 abnormal core temperature curves at an earlier stage. Monitoring core body temperature in real  
217 time on a continuous basis might be very useful in cases of factitious fevers, chronic infections  
218 and fevers of unknown origin. Non aggressive, continuous real time recording of the body  
219 temperature during infection offers a new tool to study the relationship between temperature  
220 and the infectious process [31]. However, ingestible telemetric body core temperature sensors  
221 have some limitations: the main one being the gastrointestinal transit time, as transit time varies  
222 for each individual due to age, gender, diet and pathology. The variability of the transit time  
223 ranges from 0.52 day to 5.6 days and the mean transit time is  $2 \pm 1.5$  days [32]. This resulted  
224 in missing measurements in our study, due to the absence of indications from the capsule.  
225 However, if needed, capsules can be prescribed every three days and the monitor can follow  
226 four capsules at the same time. Another inconvenience was the exclusion of patients who might  
227 require an MRI scan, who represented 15% of febrile patients in our cohort. However, one final  
228 positive aspect of this type of measurement is that, in our experience, the time spent by the  
229 nurse waiting for axillary temperature readings was calculated in our study as  $2.83 \pm 0.66$   
230 minutes. The cumulated time spent by nurses waiting to collect axillary temperature readings  
231 in our study was estimated at 12.26 hours. Although a full medico-economic study is required,  
232 it is likely that the capsule would save time.

233

## 234 **Conclusions**

235 Of existing temperature measurement sensors, only the ingestible capsule has a good  
236 correlation and agreement with axillary temperature measurement. It is sufficiently reliable to  
237 adequately estimate the body temperature in clinical care. In addition, the capsules offer real-  
238 time measurement (every 30 seconds, one minute, two minutes or five minutes). The number  
239 of collection points, its non-invasiveness, and the remote control in real time offer new  
240 opportunity for future investigation of fevers during the course of infectious diseases.

241

## 242 **Acknowledgments**

243 We would like to thank the nurses and the medical team from the University Hospital Institute  
244 Méditerranée-Infection who have been very helpful. We also thank all the patients for their  
245 willingness to participate in this study.

246 The English language in this text was edited by by Tradonline ®. Plagiarism was tested by  
247 Urkund®.

248

249 **Footnotes**

250 **Contributors**

251 Conceived and designed the experiments: PB, FH, CM. Performed the experiments: FH.

252 Analysed the data: FH, CM. Wrote the paper: FH, PB.

253 **Financial support**

254 This work was supported by ANR “Investissements d’avenir”, Méditerranée infection 10-

255 IAHU-03. Ingestible capsule sensors, monitor and e-tact sensors were provided by BodyCap©,

256 e-Celsius performance© thanks to Sébastien Moussay.

257 **Conflict of Interest**

258 All authors are no reported conflicts of interest. All authors have submitted the ICMJE Form

259 for Disclosure of Potential Conflicts of Interest. Conflicts that the editors consider relevant to

260 the content of the manuscript have been disclosed.

261

262

## 263 **References**

- 264 1. Marui S, Misawa A, Tanaka Y, Nagashima K. Assessment of axillary temperature for the  
265 evaluation of normal body temperature of healthy young adults at rest in a thermoneutral  
266 environment. *J Physiol Anthropol.* 22 févr 2017;36(1):18.
- 267 2. Bindu B, Bindra A, Rath G. Temperature management under general anesthesia: Compulsion or  
268 option. *J Anaesthesiol Clin Pharmacol.* 2017;33(3):306-16.
- 269 3. Young PJ, Saxena M. Fever management in intensive care patients with infections. *Crit Care.*  
270 2014;18(2):206.
- 271 4. Arnow PM, Flaherty JP. Fever of unknown origin. *Lancet.* 23 août 1997;350(9077):575-80.
- 272 5. Robinson JL, Seal RF, Spady DW, Joffres MR. Comparison of esophageal, rectal, axillary,  
273 bladder, tympanic, and pulmonary artery temperatures in children. *J Pediatr.* oct  
274 1998;133(4):553-6.
- 275 6. Kimberger O, Thell R, Schuh M, Koch J, Sessler DI, Kurz A. Accuracy and precision of a novel  
276 non-invasive core thermometer. *Br J Anaesth.* août 2009;103(2):226-31.
- 277 7. Fox RH, Solman AJ, Isaacs R, Fry AJ, MacDonald IC. A new method for monitoring deep body  
278 temperature from the skin surface. *Clin Sci.* janv 1973;44(1):81-6.
- 279 8. Niven DJ, Gaudet JE, Laupland KB, Mrklas KJ, Roberts DJ, Stelfox HT. Accuracy of peripheral  
280 thermometers for estimating temperature: a systematic review and meta-analysis. *Ann Intern Med.*  
281 17 nov 2015;163(10):768-77.
- 282 9. Byrne C, Lim CL. The ingestible telemetric body core temperature sensor: a review of validity  
283 and exercise applications. *British Journal of Sports Medicine.* 1 mars 2007;41(3):126-33.

- 284 10. Chapon PA, Gauthier A, Bulla J, Moussay S. Calibration and performance assessment of a  
285 temperature sensor prototype using a 1-point calibration procedure. *Rev Sci Instrum.* nov  
286 2012;83(11):114907.
- 287 11. Bongers CCWG, Daanen HAM, Bogerd CP, Hopman MTE, Eijsvogels TMH. Validity,  
288 Reliability, and Inertia of Four Different Temperature Capsule Systems. *Med Sci Sports Exerc.*  
289 janv 2018;50(1):169-75.
- 290 12. Bogerd CP, Velt KB, Annaheim S, Bongers CCWG, Eijsvogels TMH, Daanen HAM.  
291 Comparison of two telemetric intestinal temperature devices with rectal temperature during  
292 exercise. *Physiol Meas.* 29 mars 2018;39(3):03NT01.
- 293 13. Fuhrman C, Chouaïd C. Concordance de deux variables : les approches numériques: Concordance  
294 entre observations qualitatives -coefficient kappa-, concordance entre méthodes quantitatives.  
295 *Revue des Maladies Respiratoires.* 1 févr 2004;21(1):123-5.
- 296 14. Koo TK, Li MY. A Guideline of Selecting and Reporting Intraclass Correlation Coefficients for  
297 Reliability Research. *J Chiropr Med.* juin 2016;15(2):155-63.
- 298 15. Bland JM, Altman DG. Agreement between methods of measurement with multiple observations  
299 per individual. *J Biopharm Stat.* 2007;17(4):571-82.
- 300 16. Gibson TM, Redman PJ, Belyavin AJ. Prediction of oesophageal temperatures from core  
301 temperatures measured at other sites in man. *Clin Phys Physiol Meas.* nov 1981;2(4):247-52.
- 302 17. Charafeddine L, Tamim H, Hassouna H, Akel R, Nabulsi M. Axillary and rectal thermometry in  
303 the newborn: do they agree? *BMC Res Notes.* 31 août 2014;7:584.
- 304 18. Sollai S, Dani C, Berti E, Fancelli C, Galli L, de Martino M, et al. Performance of a non-contact  
305 infrared thermometer in healthy newborns. *BMJ Open.* 16 mars 2016;6(3):e008695.

- 306 19. Osio CE, Carnelli V. Comparative study of body temperature measured with a non-contact  
307 infrared thermometer versus conventional devices. The first Italian study on 90 pediatric patients.  
308 *Minerva Pediatr.* août 2007;59(4):327-36.
- 309 20. Teran CG, Torrez-Llanos J, Teran-Miranda TE, Balderrama C, Shah NS, Villarroel P. Clinical  
310 accuracy of a non-contact infrared skin thermometer in paediatric practice. *Child Care Health*  
311 *Dev.* juill 2012;38(4):471-6.
- 312 21. Apa H, Gözmen S, Bayram N, Çatkoğlu A, Devrim F, Karaarslan U, et al. Clinical accuracy of  
313 tympanic thermometer and noncontact infrared skin thermometer in pediatric practice: an  
314 alternative for axillary digital thermometer. *Pediatr Emerg Care.* sept 2013;29(9):992-7.
- 315 22. Chan L-S, Cheung GTY, Lauder IJ, Kumana CR. Screening for Fever by Remote-sensing Infrared  
316 Thermographic Camera. *Journal of Travel Medicine.* 1 sept 2004;11(5):273-9.
- 317 23. Kiekkas P, Stefanopoulos N, Bakalis N, Kefaliakos A, Karanikolas M. Agreement of infrared  
318 temporal artery thermometry with other thermometry methods in adults: systematic review. *J Clin*  
319 *Nurs.* avr 2016;25(7-8):894-905.
- 320 24. Mogensen CB, Wittenhoff L, Fruerhøj G, Hansen S. Forehead or ear temperature measurement  
321 cannot replace rectal measurements, except for screening purposes. *BMC Pediatr* [Internet]. 26  
322 janv 2018 [cité 21 févr 2018];18. Disponible sur:  
323 <https://www.ncbi.nlm.nih.gov/pmc/articles/PMC5787302/>
- 324 25. Fortuna EL, Carney MM, Macy M, Stanley RM, Younger JG, Bradin SA. Accuracy of non-  
325 contact infrared thermometry versus rectal thermometry in young children evaluated in the  
326 emergency department for fever. *J Emerg Nurs.* mars 2010;36(2):101-4.
- 327 26. Hausfater P, Zhao Y, Defrenne S, Bonnet P, Riou B. Cutaneous infrared thermometry for  
328 detecting febrile patients., *Cutaneous Infrared Thermometry for Detecting Febrile Patients.* *Emerg*  
329 *Infect Dis.* août 2008;14, 14(8, 8):1255, 1255-8.

- 330 27. Rastgar-Jazi M, Mohammadi F. Parameters sensitivity assessment and heat source localization  
331 using infrared imaging techniques. *BioMedical Engineering OnLine*. 21 sept 2017;16:113.
- 332 28. Roxane B, Ouma Chandrou K, Pierre Alexandre C, Christophe C, Bruno S, Stéphane B, et al.  
333 Gastrointestinal thermal homogeneity and effect of cold water ingestion. *Journal of Thermal*  
334 *Biology*. déc 2018;78:204-8.
- 335 29. Domitrovich JW, Cuddy JS, Ruby BC. Core-Temperature Sensor Ingestion Timing and  
336 Measurement Variability. *J Athl Train*. 2010;45(6):594-600.
- 337 30. Drewry AM, Fuller BM, Bailey TC, Hotchkiss RS. Body temperature patterns as a predictor of  
338 hospital-acquired sepsis in afebrile adult intensive care unit patients: a case-control study. *Crit*  
339 *Care*. 2013;17(5):R200.
- 340 31. Plaza JJG, Hulak N, Zhumadilov Z, Akilzhanova A. Fever as an important resource for  
341 infectious diseases research. *Intractable & Rare Diseases Research*. 25 avr 2016;5(2)(97-102):6.
- 342 32. McKenzie JE, Osgood DW. Validation of a new telemetric core temperature monitor. *Journal of*  
343 *Thermal Biology*. 2004;7-8(29):605-11.
- 344

1 **Figure legends**

2 **Figure 1. Time trend data**

3 **A**, Time trend data of all measurements in one selected patient with acute community acquired  
4 pneumonia. Black squares represent axillary temperature measurements; red points represent  
5 ingestible capsule temperature measurements; green stars represent non-contact temperature  
6 measurements; blue points represent eTact temperature measurements. **B**, Time trend data of a  
7 patient with hypothermia.

8 **Figure 2. Regression line between the axillary temperature measurements ( $T_{axi}$ ) and non-**  
9 **contact forehead temperature measurements ( $T_{no-c}$ ), ingestible capsule temperature**  
10 **measurements ( $T_{cap}$ ) as well as eTact temperature measurements ( $T_{etac}$ ). With 95%**  
11 **confidence interval.**

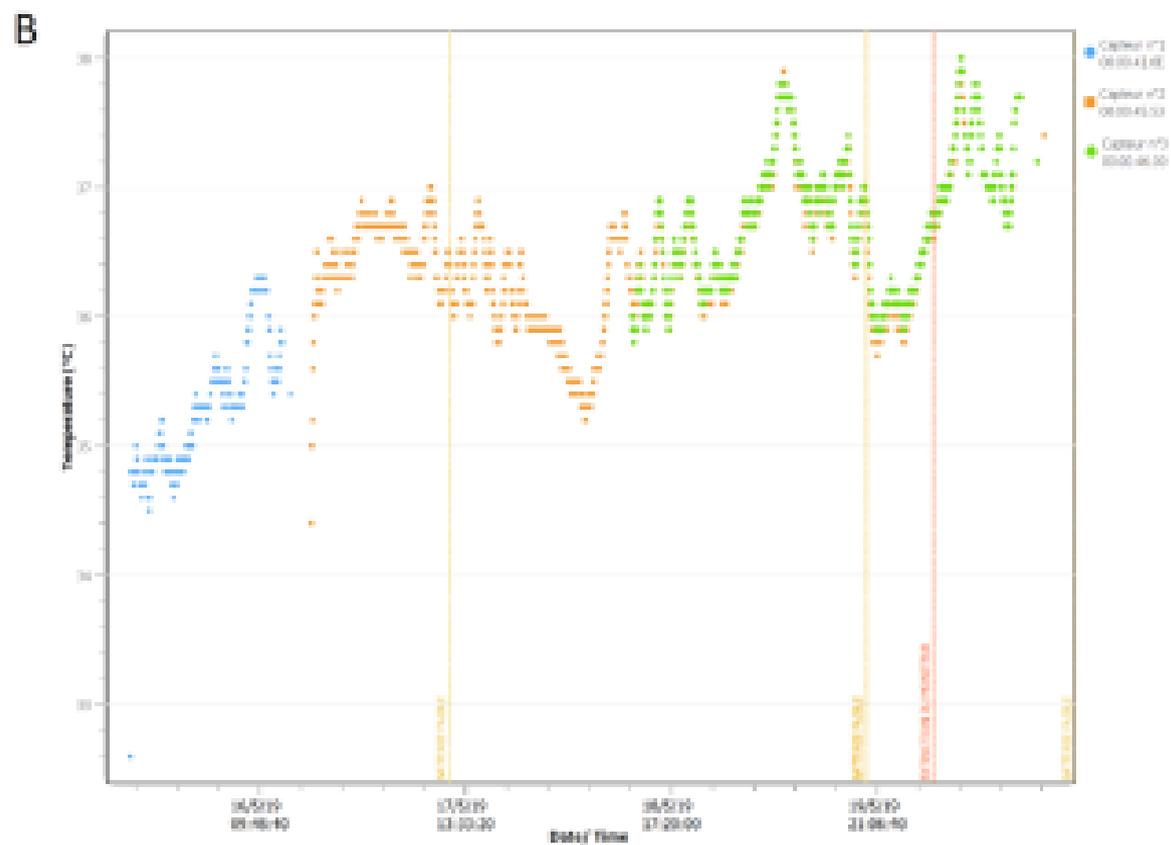
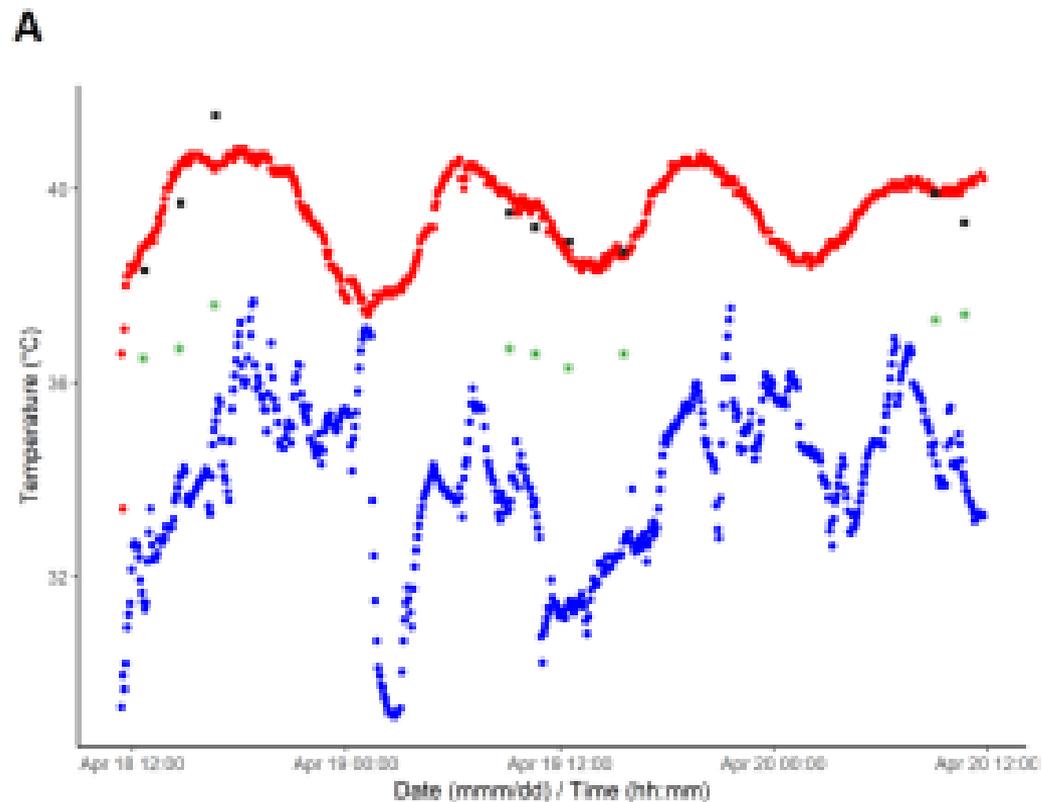
12 **A**, Regression line between the  $T_{axi}$  and  $T_{no-c}$  ( $r=0.47$ ,  $p<0.001$ ). **B**, Regression line between  
13 the  $T_{axi}$  and  $T_{cap}$ . ( $r=0.85$ ,  $p<0.001$ ). **C**, Regression line between the  $T_{axi}$  and  $T_{etac}$  ( $r=0.42$ ,  
14  $p<0.001$ ).

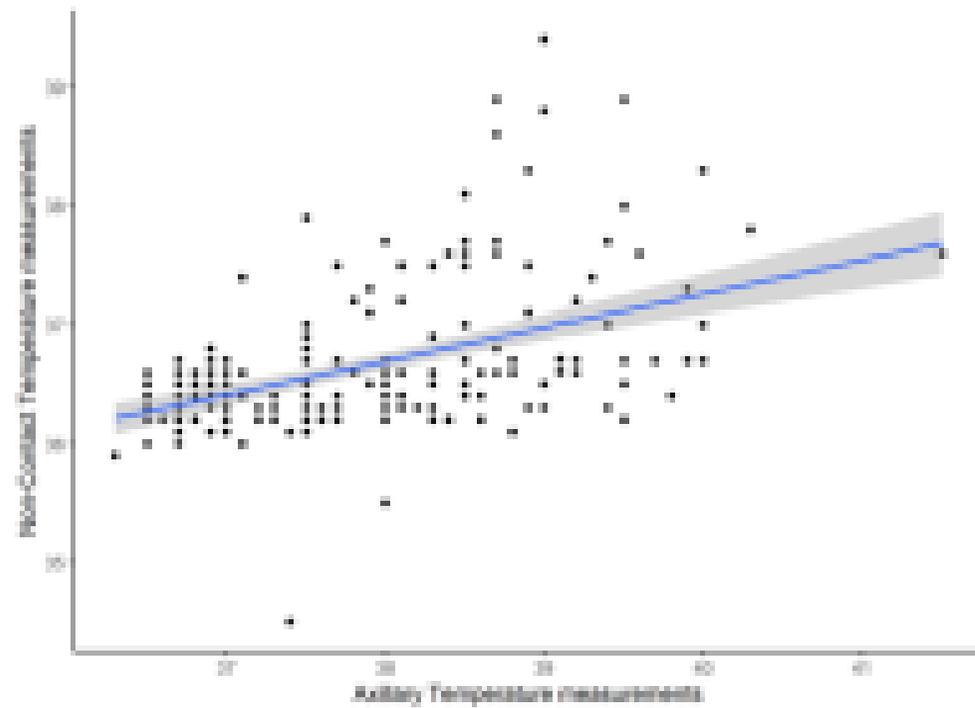
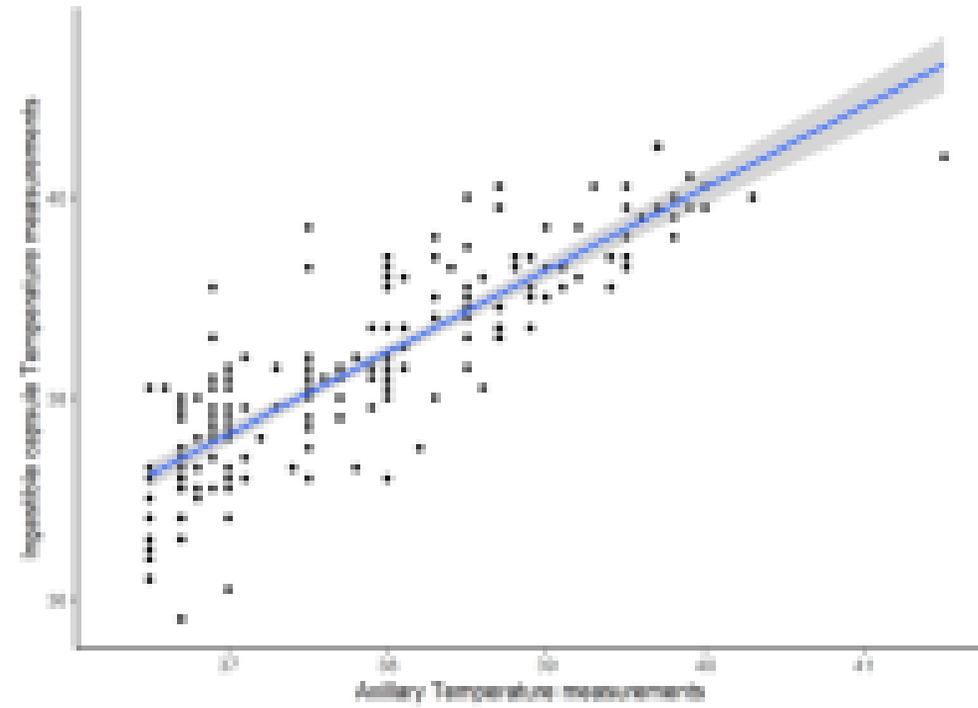
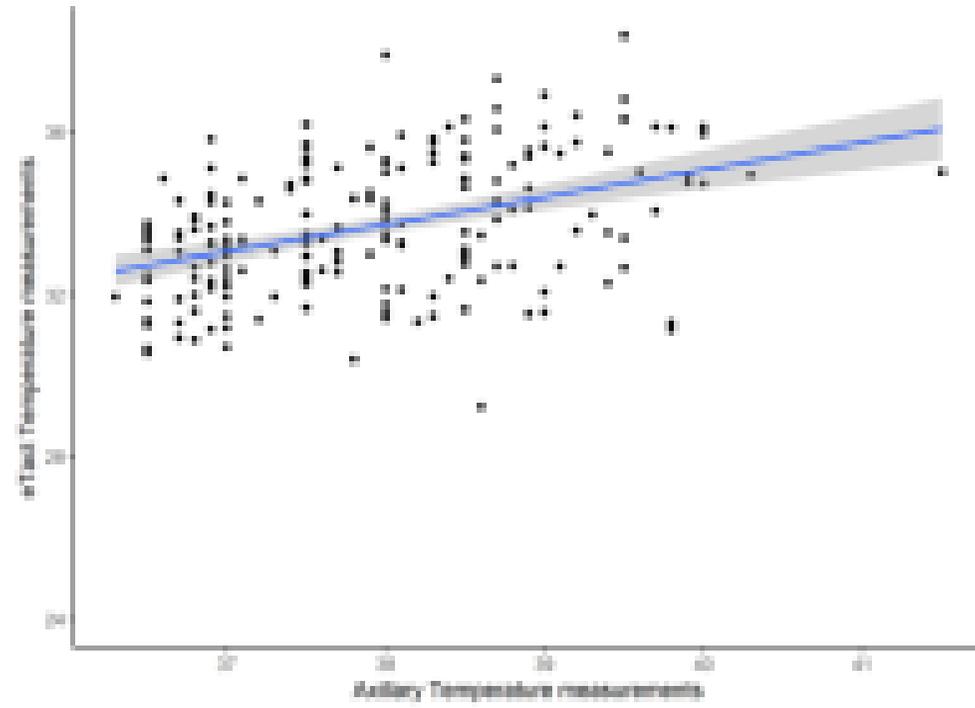
15 **Figure 3. Bland-Altman plot. Comparison of the difference between two measurements**  
16 **with the 95% limits of agreement. The red line represents the mean difference between**  
17 **two measurements, with 95% confidence interval (two grey dashed lines). Blue lines**  
18 **represent the upper and lower limits of agreement and grey dashed lines represent their**  
19 **95% confidence interval.**

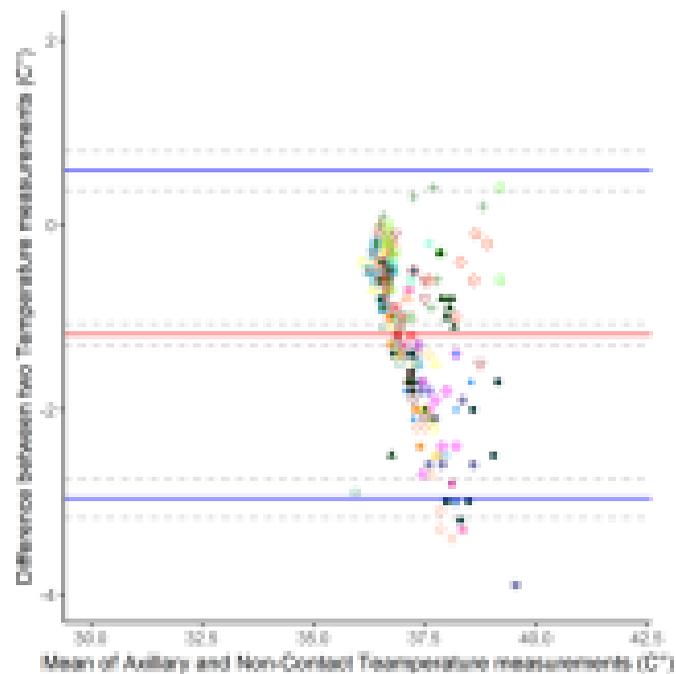
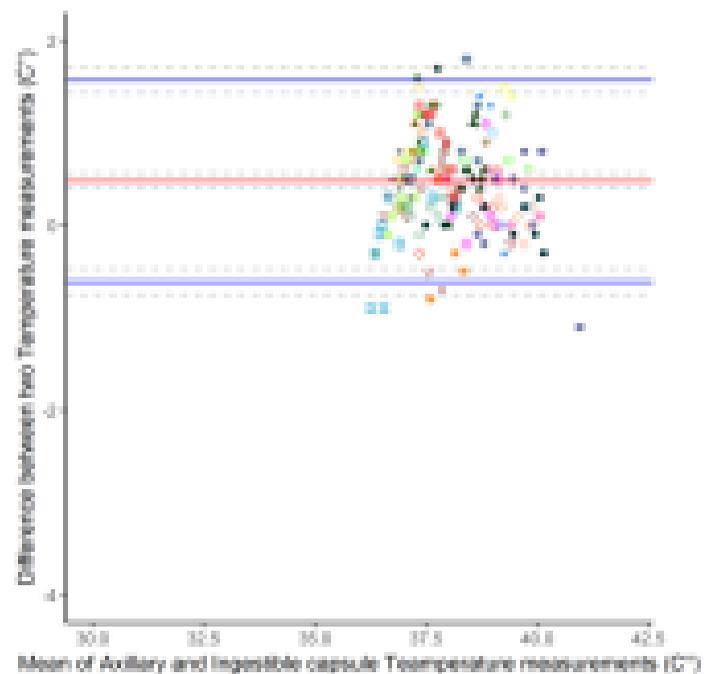
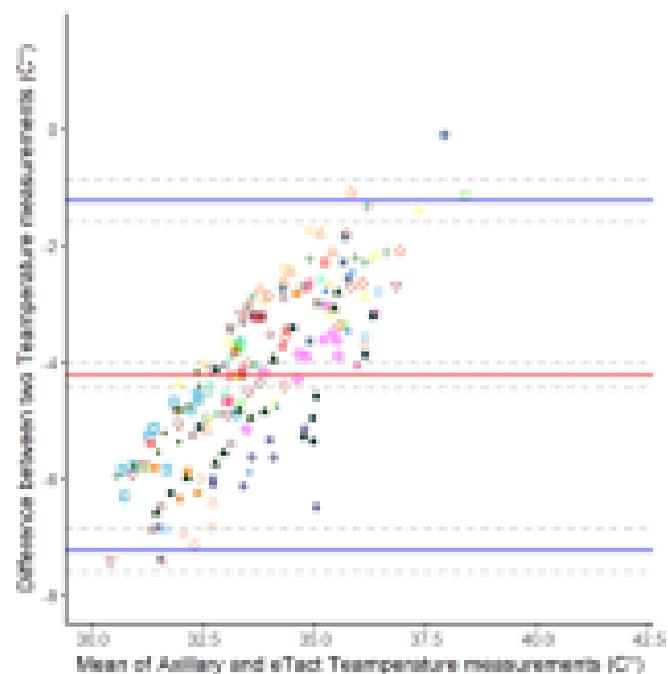
20 **A**, Comparison of the difference between the  $T_{axi}$  and  $T_{no-c}$ . The mean difference between  
21  $T_{axi}$  vs.  $T_{no-c}$  ( $-1.18^{\circ}\text{C}$ ). The upper and lower limits of agreement ( $-2.96^{\circ}\text{C}$  and  $0.58^{\circ}\text{C}$ ). **B**,  
22 Comparison of the difference between the  $T_{axi}$  and  $T_{cap}$ . The mean difference between  $T_{axi}$  vs.  
23  $T_{cap}$  ( $0.48^{\circ}\text{C}$ ). The upper and lower limits of agreement ( $-0.60^{\circ}\text{C}$  and  $1.56^{\circ}\text{C}$ ). **C**, Comparison

24 of the difference between the  $T_{axi}$  and  $T_{etac}$ . The mean difference between  $T_{axi}$  vs  $T_{etac}$  (-  
25 4.23°C). The upper and lower limits of agreement (-7.22°C and -1.23°C).

26



**A****B****C**

**A****B****C****Patients**

- Patient 1      ○ Patient 16
- Patient 2      ○ Patient 18
- Patient 3      ○ Patient 17
- Patient 4      ○ Patient 18
- Patient 5      ○ Patient 19
- Patient 6      ○ Patient 19
- Patient 7      ○ Patient 20
- Patient 8      ○ Patient 21
- Patient 9      ○ Patient 22
- Patient 10      ○ Patient 23
- Patient 11      ○ Patient 24
- Patient 12      ○ Patient 25
- Patient 13      ○ Patient 26
- Patient 14

## 1 Tables

2 **Table 1. Characteristics of the 26 patients.** This table shows patient demography, medication  
3 and medical history.

Sex	n	(%)
Female	12	(46.2)
Male	14	(53.8)
Baseline	mean	(SD)
Age (years)	48.6	(17.5)
Body weight (kg)	65.9	(13.66)
Blood pressure (mm Hg)		
Systolic pressure	118.6	(17.87)
Diastolic pressure	64.3	(12.98)
Pulse (bpm)	95.4	(15.5)
Body temperature during inclusion (°C)	38.73	(0.74)
Capsule transit time (hours)	37.3	(14.8)
Treatments	n	(%)
Antibiotics	19	(33.92)
Antipyretic	8	(14.28)
Antivirus	4	(7.14)
Antimalarial	1	(1.78)
Other	24	(42.85)
Medical history	n	(%)
Surgical	7	(19.44)
Cardiovascular	8	(22.22)
Metabolic disorders	6	(16.66)
Pulmonary	2	(5.55)

---

Urinary	2	(5.55)
Gastro-intestinal	3	(8.33)
Infectious	8	(22.22)

---

4

5

6 **Table 2. Descriptive statistics of axillary temperature, non-contact temperature, ingestible**  
7 **capsule temperature and eTact temperature measurements during 48-hour observation**  
8 **period.**

	Total N (measurement points)	Valid N	Missing (n, %)	Mean (°C)	Standard Deviation	Max (°C)	Mini (°C)
Axillary temperature (T <sub>axi</sub> )	255	213	42 (16.5)	37.84	1.02	41.5	36.3
Non-contact forehead temperature (T <sub>no-c</sub> )	255	216	39 (15.3)	36.66	0.61	39.4	34.5
Ingestible capsule temperature (T <sub>cap</sub> )	255	213	42 (16.5)	38.26	1.01	40.5	35.7
eTact temperature (T <sub>tac</sub> )	255	225	30 (11.8)	33.59	1.84	38.37	24.03

9

10

11 **Table 3. Analyses of correlation (Pearson) and agreement (Intraclass Correlations) among**  
 12 **three different devices and axillary temperature measurements.**

	Correlation coefficient				Agreement		
	Pearson(r)	95% CI	sig.	R <sup>2</sup>	ICC	95% CI	sig.
Non-contact forehead (Tno-c )	0.47	0.36;0.57	p<0.001	0.22	0.3445	-0.18; 0.63	p<0.001
Ingestible capsule (Tcap )	0.85	0.81;0.98	p<0.001	0.72	0.8730	0.55; 0.94	p<0.001
eTact (Tetac )	0.42	0.30;0.52	p<0.001	0.17	0.1229	-0.09; 0.37	p<0.001

13

14

15 **Table 4. Detail of Bland-Altman plot among three different devices and axillary**  
 16 **temperature measurements.**

	Mean Difference (°C)	Standard Deviation	Std. Error Mean	95% Confidence Interval of the Difference (°C)		limits of agreement ( $d \pm 1.96SD$ ) (°C)	
				Lower	Upper	Lower	Upper
				Tno-c vs. Taxi	-1.1892	0.9049	0.062
Tcap vs. Taxi	0.4804	0.5549	0.0409	0.3997	0.5611	-0.6071	1.5680
Tetac vs. Taxi	-4.2316	1.5285	0.1091	-4.4470	-4.0163	-7.2277	-1.2356

17

18